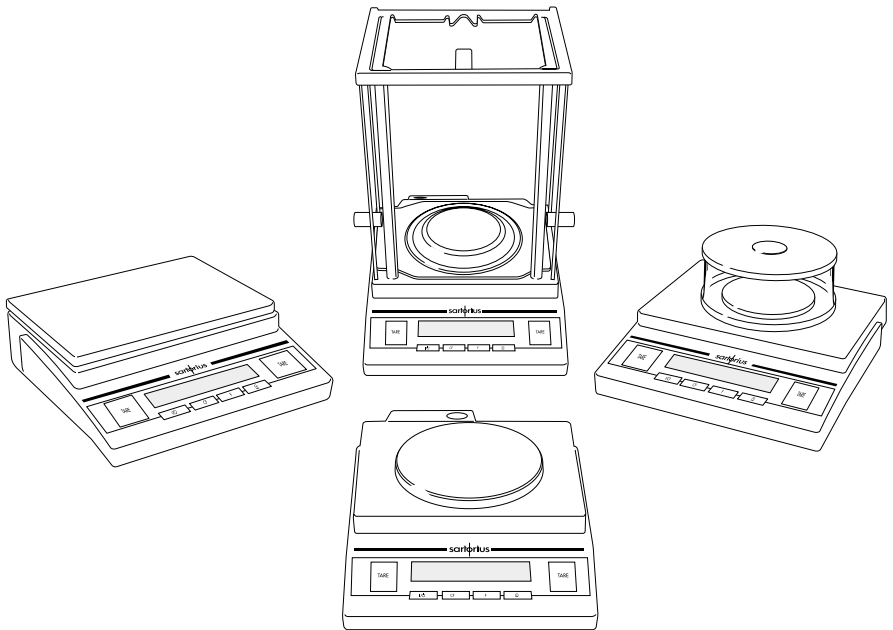


Sartorius Basic^{lite} Series Sartorius Gem^{lite} Series

Electronic Precision Balances
and Precious Metal Scales

Operating Instructions



Practical Use

The Basic^{lite} Series and Gem^{lite} Series from Sartorius offer precision balances/scales with capacities ranging from 0.1 mg to 12 kg.

These balances/scales meet the highest requirements on the accuracy and reliability of weighing results through the following features:

- Efficient filtering-out of unfavorable ambient conditions such as vibrations, drafts, etc.
- Stable and reproducible results
- Rugged, durable weighing system

Basic^{lite} balances and Gem^{lite} scales save work and speed up simple routine applications through:

- Ultrafast response times
- Easy operation

You can also choose from the following extra functions for simple applications:

- Toggling between weight units
- Net-total formulation (tare memory)
- Counting
- Weighing in percent
- Averaging

Warning and Safety Information

Read these operating instructions thoroughly before using your balance/scale to prevent damage to the equipment. Keep these instructions in a safe place.

Follow the instructions below to ensure safe and trouble-free operation of your balance/scale:

- ⚠ Make sure that the voltage rating printed on the AC adapter is identical to your local line voltage
- ⚠ Use only a commercially available 9-volt battery or rechargeable battery

Contents

| | |
|--|----|
| Practical Use | 2 |
| Contents | 2 |
| Warning and Safety Information | 2 |
| Getting Started | 3 |
| Operating the Balance/Scale | |
| Basic Weighing Function | 8 |
| Calibration/Adjustment | 9 |
| Application Programs | |
| Counting | 10 |
| Weighing in Percent | 12 |
| Weigh Averaging | 14 |
| Net-Total Formulation/ Second Tare Memory | 16 |
| Toggle Between Weighing Units | 17 |
| Configuring the Balance/Scale | |
| Setting the Parameters (Menu Codes) | 18 |
| Balance/Scale Operating Menu (Overview) | 19 |
| Error Codes | 20 |
| Care and Maintenance | 21 |
| Instructions for Recycling | 22 |
| Overview | |
| Specifications | 23 |
| Accessories (Options) | 27 |
| CE Marking | 28 |

- ⚠ Do not use this balance/scale in a hazardous area/location
- The only way to turn the power off completely is to disconnect the AC adapter
- Connect only Sartorius accessories and options, as these are optimally designed for use with your balance/scale.
- Protect the AC adapter from contact with liquid.

Do not open the balance/scale housing. If the seal is broken, this will result in forfeiture of all claims under the manufacturer's warranty.

Getting Started

Warranty

Do not miss out on the benefits of our full warranty. Please contact your local Sartorius office or dealer for further information. Complete the warranty registration card, if available indicating the date of installation, and return the card to your Sartorius office or dealer.

Storage and Shipping Conditions

Do not expose the balance/scale to shocks, vibration, moisture or extreme temperatures.

Unpacking the Balance/Scale

- After unpacking the balance/scale, check it immediately for any visible damage as a result of rough handling during shipment.
- If you see any sign of damage, proceed as directed in the chapter entitled "Care and Maintenance," under the section on "Safety Inspection."

Save the box and all parts of the packaging until you have successfully installed your balance/scale. Only the original packaging provides the best protection for shipment. Before packing your balance/scale, unplug all connected cables to prevent damage.

Equipment Supplied

The equipment supplied includes the components listed below:
BL210S, BL120S, BL60S, GC503, GC103

- Balance/scale
- Weighing pan
- Pan support
- Shield ring
- Shield plate
- Dust cover
- AC adapter
- Gem tray (only with GC models)
- Calibration weight 100 g, F1 (only with model GC503)

BL150S

- Balance/scale
- Weighing pan
- Pan support
- Glass draft shield with cover
- AC adapter

Balances/scales with a readability of ≥ 0.01 g

- Balance/scale
- Weighing pan
- Pan support (only on models with a round weighing pan)
- AC adapter

Installation Instructions

Your balance/scale is designed to provide reliable weighing results under normal ambient conditions. When choosing a location to set up your balance/scale, observe the following so that you will be able to work with added speed and accuracy:

- Set up the balance/scale on a stable, even surface
- Avoid placing the balance/scale in close proximity to a heater or otherwise exposing the balance/scale to heat or direct sunlight
- Protect the balance/scale from drafts that come from open windows or doors
- Avoid exposing the balance/scale to extreme vibrations during weighing
- Protect the balance/scale from aggressive chemical vapors
- Do not expose the balance/scale to extreme moisture over long periods

Conditioning the Balance/Scale:


Moisture in the air can condense on the surfaces of a cold balance/scale whenever it is brought into a substantially warmer place. If you transfer the balance/scale to a warmer area, make sure to condition it for about 2 hours at room temperature, leaving it unplugged from AC power.

Information on Radio Frequency Interference

Warning!

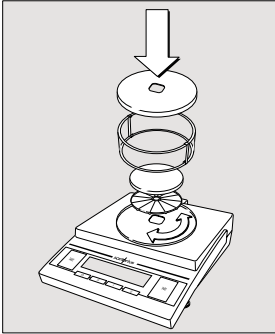
This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause interference to radio communications. It has been tested and found to comply with the limits for a Class A computing device pursuant to Subpart J of Part 15 of FCC Rules, which are designed to provide reasonable protection against such interference, when operated in a commercial environment. Operation of this equipment in a residential area is likely to cause interference, in which case the user, at his own expense, will be required to take whatever measures may be required to correct the interference.

Setting up the Balance/Scale



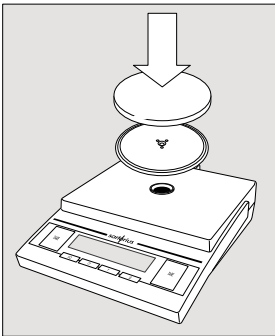
Balances/Scales with an Analytical Draft Shield Chamber:

- Place the components listed below inside the chamber in the order given:
 - Shield plate
 - Shield ring
 - Pan support
 - Weighing pan
 - Gem tray (only with GC models)



Balances/Scales with a Glass Draft Shield:

- Place the components listed below inside the chamber in the order given:
 - Draft shield base – place it on the balance so that the edge for fitting the glass draft shield faces upwards and turn it until it is firmly in place
 - Pan support
 - Weighing pan
 - Glass draft shield
 - Draft shield cover – place it on the balance so that the edge faces downwards




Balances/Scales with a Round Weighing Pan

- Place the components listed below inside the chamber in the order given:
 - Pan support
 - Weighing pan

Balances/Scales with a Rectangular Weighing Pan:

- Place the weighing pan on the balance/scale



Connecting the Balance/Scale to AC Power/ Safety Precautions

Use only original Sartorius AC adapters:


- for Europe: 6971948 – for the RSA: 6971949
- for the U.S.: 6971947 – for Australia: 6971950

- Insert the right-angle plug into the jack
- The AC adapter rated to Class 2 can be plugged into any wall outlet without requiring any additional safety precautions

The ground is connected to the balance/scale housing, which can be additionally grounded for operation.

Using a Non-Rechargeable/Rechargeable Battery

(not for models BL210S, BL120S, BL60S, BL150S, BL1500S, GC503, GC103, GM1502)




- A non-rechargeable or rechargeable battery is not included with the equipment supplied

⚠ Use only a commercially available non-rechargeable or rechargeable 9-volt battery

⚠ When using a rechargeable battery, always use an external charger to recharge the battery

- Lay the balance/scale on its side
- Open the battery compartment:
Lift the compartment cover




- Insert the 9-volt (rechargeable) battery in the compartment

- Make sure to connect the positive and negative poles correctly

⚠ All used batteries are classified as waste that requires special handling (not "household" waste). Dispose of rechargeable batteries in accordance with the applicable special waste disposal regulations.

- Close the battery compartment:
Press down on the cover until it clicks into place

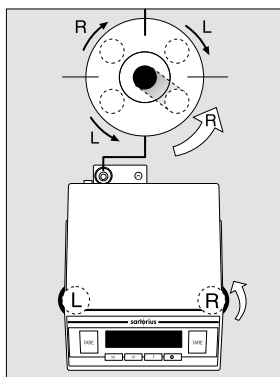


Selecting the Line Voltage (Mains Voltage)

Use the following original AC adapters for selecting the line voltage:

- AC adapter TNG8, order no. 6971951 (universal)
- or
- AC adapter TNG8, order no. 6971952 (for the U.K.)

- Use the switch to toggle between 230 V and 115 V




Leveling the Balance/Scale

(only for models BL210S, BL120S, BL60S, BL150S, BL1500S, GC503, GC103, GM1502)

Level the balance/scale any time you set it up in a new location. Use only the 2 front feet of the balance/scale for leveling.

- Turn the 2 rear feet until they are in position (only on models BL1500S and GM1502)
 - Turn the 2 front feet as shown here in the illustration until the air bubble is centered in the level indicator
- > In most cases, this will require several adjustment steps



Anti-theft Locking Device

To protect against theft, use the mounting lug on the rear panel of the balance/scale.

- Secure the balance/scale at the place of installation, for example with a chain or a lock



Operating the Balance/Scale

Basic Weighing Function

Available Features

- Taring the balance/scale
You can tare the balance/scale within the entire weighing range.

Preparation

- Turn on the balance/scale: Press 
- To change configurations: See the chapter entitled "Configuring the Balance/Scale"
- To load factory-set configurations:
See "Configuring the Balance/Scale," parameter 9 – 1
- To tare the balance/scale: Press 






Additional Functions

- To turn off the balance/scale: Press 

Example

Basic weighing

Menu code settings: Factory-set codes

| Step | Key (or instruction) | Display/Printout |
|---|---|---|
| 1. Turn on the balance/scale |  | |
| | Self-test is performed |  |
| 2. Place container on balance/scale (here: 52 g) |  | + 52.0 g |
| 3. Tare the balance/scale |  | + 0.0 g |
| 4. Place sample in container on balance/scale (here: 150.2 g) |  | + 150.2 g |

Calibration/Adjustment*

Always calibrate/adjust the balance/scale after setting it up in a new location.

Available Features

Calibration/adjustment can only be performed when

- there is no load on the balance/scale,
- the balance/scale is tared,
- the internal signal is stable.

If these conditions are not met, an error message is displayed.

The weight required for calibration/adjustment is displayed (see "Accessories" for calibration weights; for model GC503 see "Equipment Supplied").







On Basic^{lite} balances, calibration/adjustment can be performed with any of three weight units: g, kg**, or lb (menu code 1.4.x)

Factory setting: Grams (menu code 1.4.1)

Example

Calibrate the balance/scale

Menu code settings: Factory-set codes

| Step | Key (or instruction) | Display/Printout |
|--|---|--|
| 1. Turn on the balance/scale |  |  |
| 2. Tare the balance/scale |  | 0.0 g |
| 3. Begin calibration |  >2 sec. | + 1000.0 |
| Calibration weight is displayed without weight unit (here: 1000 g) | | |
| 4. Place the indicated calibration weight on the balance/scale |  | 1000.0 |
| After calibration, the calibration weight is displayed with wt. unit | | + 1000.0 g |
| 5. Remove the calibration weight |  | 0.0 g |

* "Calibration" technically means to determine the difference between the balance/scale readout and the actual weight on the pan to determine the accuracy.

Adjustment means to bring a balance/scale into the state of accuracy required for its use.

Therefore, "calibration," as used in this manual, actually means "adjustment."

** = not on models with a readability of 0.1 mg

Application Programs

Counting

Purpose

With the Counting program you can determine the number of parts that each have approximately equal weight.

Available Features

- Store the current weight value to have it loaded as the preset reference sample quantity next time you initialize the Counting application
- The reference sample quantity can be changed in the operating menu:
See "Configuring the Balance/Scale"
- The average piece weight is automatically output via the optional data interface port after initialization, if the menu code for "Printout with data ID codes" is set
- Press **[F]** to toggle the display between piece count and weight

Factory Settings

Reference sample quantity: 10 (menu code **3.3.2**)

Preparation

- Configure the Counting application in the operating menu:
See "Configuring the Balance/Scale"
Menu code **2.1.4** Counting
- Reference sample quantity:
Menu code **3.3.1** 5 pcs
Menu code **3.3.2** 10 pcs
Menu code **3.3.3** 20 pcs
Menu code **3.3.4** 50 pcs
Menu code **3.3.5** 100 pcs

See also "Configuring the Balance/Scale"












Example

Determine an unknown piece count; weigh the preset reference sample quantity

Settings (changes in the factory settings required for this example):

Menu: Application program: Counting (menu code 2. 1. 4)

Reference sample quantity: 20 pcs (menu code 3. 3. 3)

| Step | Key (or instruction) | Display/Printout |
|--|---|--|
| 1. Turn on the balance/scale |  |  |
| 2. Tare the balance/scale |  | 0.0 g |
| 3. Display the reference sample quantity (here: 20 pcs) |  >2 sec. | rEF 20 (briefly) |
| 4. Place the reference sample quantity (20 pcs) on the balance/scale (here: 66 g) |  | + 66.0 g |
| 5. Start the application; if the print format is set to include data ID codes, the following is printed: |  | + 20 pcs wRef + 3.300 g |
| 6. Weigh uncounted parts (here: 174 pcs) |  | + 174 pcs |
| 7. Display weight |  | + 574.2 g |
| 8. Display quantity |  | + 174 pcs |
| 9. Unload the balance/scale |  | 0 pcs |
| 10. Delete the reference value |  | |
| 11. Repeat the procedure starting from step 6, if desired. | | |

Weighing in Percent

Purpose

This application program allows you to obtain weight readouts in percent which are in proportion to a reference weight.

Available Features

- Store the current weight value to have it loaded as the preset reference percentage next time you initialize the Weighing in Percent application
- The reference percentage can be changed in the operating menu:
See "Configuring the Balance/Scale"
- The reference percentage is automatically output via the optional data interface port after initialization, if the menu code for "Printout with data ID codes" is set
- Press **[F]** to toggle the display between percentage and weight

Factory Settings

Reference percentage: 10 (menu code **3.3.2**)

Preparation

- Configure the Weighing in Percent application in the operating menu:
See "Configuring the Balance/Scale"
Menu code **2.1.5** Weighing in percent

- Reference percentage:

| | |
|------------------------|-------|
| Menu code 3.3.1 | 5 % |
| Menu code 3.3.2 | 10 % |
| Menu code 3.3.3 | 20 % |
| Menu code 3.3.4 | 50 % |
| Menu code 3.3.5 | 100 % |

See also "Configuring the Balance/Scale"












Example

Determine an unknown percentage; store the weight on the balance/scale as a reference percentage

Settings (changes in the factory settings required for this example):

Menu: Application program: Weighing in percent (menu code **2. 1. 5**)

Menu: Reference percentage 100 % (menu code **3. 3. 5**)

| Step | Key (or instruction) | Display/Printout |
|--|--|--|
| 1. Turn on the balance/scale |  |  |
| 2. Tare the balance/scale |  | 0.0 g |
| 3. Display the reference percentage |  > 2 sec. | REF 100 |
| 4. Place the reference weight for 100% on the balance/scale (here: 222.5 g) |  | +222.5 g |
| 5. Start application; if the print format is set to include data ID codes, the following is printed: |  | + 100.00 % Wxx% + 222.500 g |
| 6. Place an unknown weight on the balance/scale (here: 322.5 g) |  | + 144.94 % |
| 7. Display weight |  | + 322.5 g |
| 8. Display percentage |  | + 144.94 % |
| 9. Unload the balance/scale |  | 0.00 % |
| 10. Delete the reference percentage |  | |
| 11. Repeat the procedure starting from step 6, if desired. | | |

Weigh Averaging

Purpose

Use this program to determine weights under unstable ambient conditions. In this program, the balance/scale calculates the weight as the average value from a defined number of individual weighing operations. These weighing operations are also known as "subweighing operations" or "subweighs."

Available Features

- The measured result displayed is the arithmetic mean shown in the selected weight unit; a triangle indicates that this is a calculated value
- You can set the number of subweighing operations performed in the operating menu: See "Configuring the Balance/Scale"
- Press **[F]** for at least 2 sec. to display the preset number of subweighing operations
- Press **[F]** to toggle the display between the calculated result and the weight

Factory Settings

Number of subweighs for averaging: 10 (**3.3.2**)

Preparation

- Configure the Weigh Averaging application in the operating menu:
See "Configuring the Balance/Scale"
Menu code **2.1.12** Averaging
- Number of subweighs for weigh averaging:
 - 3.3.1** 5 subweighs
 - 3.3.2** 10 subweighs
 - 3.3.3** 20 subweighs
 - 3.3.4** 50 subweighs
 - 3.3.5** 100 subweighs











See also "Configuring the Balance/Scale"

Example

Determine the weight of a sample in extremely unstable ambient conditions by calculating the average of 10 subweighing operations.

Settings (changes in the factory settings required for this example):

Menu: Application program: Weigh Averaging (menu code 2. 1. 12)

| Step | Key (or instruction) | Display/Printout |
|---|---|---|
| 1. Turn on the balance/scale |  |  |
| 2. Tare the balance/scale |  | 0.0 g |
| 3. Display the number of subweighs (here: 10) |  >2 sec. | EF 10 (briefly) |
| 4. Place sample on the balance/scale (weight readout fluctuates; here: about 275 g) |  | + 8888 |
| 5. Start measurement |  | + 8888 10 9 8 ... 1 |
| After 10 subweighs | | + 275.5 g  |
| If the print format is set to include data ID codes, the following is printed: | | RES + 275.5 g |
| 6. Unload the balance/scale |  | + 275.5 g  (stable display) |
| 7. Delete the result |  | |
| 8. Repeat the procedure starting from step 4, if desired. | | |

Net-Total Formulation/Second Tare Memory










With this application program you can weigh in components for formulation of a mixture.

Preparation

Configure the Net-Total Formulation/Second Tare Memory application in the operating menu: See "Configuring the Balance/Scale"

Menu code **2.13**

Example

| Step | Key (or instruction) | Display/Printout |
|---|---|---|
| 1. Turn on the balance/scale |  |  |
| 2. Place an empty container on the balance/scale |  | + 65.0 g |
| 3. Tare the balance/scale |  | |
| 4. Add the first component |  | + 120.5 g |
| 5. Store the first component weight If the print format is set to include data ID codes, the following is printed: |  | 0.0 g _{NET} |
| 6. Add the next component |  | N1 + 120.5 g |
| 7. Store the 2nd component weight |  | 0.0 g _{NET} |
| 8. Add further components, if desired | As described for steps 5 and 6 | |
| 9. Display total weight and fill to desired final weight |  | + 191.0 g |

Toggle Between Weight Units

With this application program you can toggle the display of a weight value back and forth between two weight units.

Configure the "Toggle Weight Units" application in the operating menu:
See "Configuring the Balance/Scale," menu code **2.1.2** Toggle weight units
(Factory setting on Gem^{lite} models)

| Menu code | | Unit | Conversion factor | Abbr. on printout |
|---------------------|---------------------|--|-------------------|-------------------|
| 1.7.1 | 3.1.1 | Taiwanese taels ⁴⁾ (only selectable on Gem ^{lite} scales) | 0.02666666000 | o |
| 1.7.2 o | 3.1.2 o | Grams | 1.00000000000 | g |
| 1.7.3 ¹⁾ | 3.1.3 ¹⁾ | Kilograms | 0.00100000000 | kg |
| 1.7.4 ²⁾ | 3.1.4 | Carats | 5.00000000000 | ct |
| 1.7.5 | 3.1.5 | Pounds | 0.00220462260 | lb |
| 1.7.6 | 3.1.6 | Ounces | 0.03527396200 | oz |
| 1.7.7 | 3.1.7 ³⁾ | Troy ounces | 0.03215074700 | ozt |
| 1.7.8 | 3.1.8 | Hong Kong taels | 0.02671725000 | tlh |
| 1.7.9 | 3.1.9 | Singapore taels | 0.02645544638 | tls |
| 1.7.10 | 3.1.10 | Taiwanese taels | 0.02666666000 | tlr |
| 1.7.11 | 3.1.11 | Grains | 15.43235835000 | GN |
| 1.7.12 | 3.1.12 | Pennyweights | 0.64301493100 | dwt |
| 1.7.13 | 3.1.13 | Milligrams | 1000.00000000000 | mg |
| 1.7.14 | 3.1.14 | Parts per pound | 1.12876677120 | /lb |
| 1.7.15 | 3.1.15 | Chinese taels | 0.02645547175 | tlc |
| 1.7.16 | 3.1.16 | Mommes | 0.26670000000 | mom |
| 1.7.17 | 3.1.17 | Austrian carats | 5.00000000000 | K |
| 1.7.18 | 3.1.18 | Tola | 0.08573333810 | tol |
| 1.7.19 | 3.1.19 | Baht | 0.06578947437 | bat |
| 1.7.20 | 3.1.20 | Mesghal | 0.21700000000 | MS |
| 1.7.22 | 3.1.22 | lb/oz – Gem ^{lite} scales only | 0.03527396200 | o |

o = Factory setting

¹⁾ = not for models with a readability of ≤ 0.2 mg

²⁾ = Factory setting only for model GC503

³⁾ = Factory setting only for GM models

⁴⁾ = Readability in increments of 1 digit

Function

- To toggle the display between the 1st and 2nd weight units:
Press the F key
















Configuring the Balance/Scale

Setting the Parameters (Menu Codes)

You can configure your Basic^{lite} balance or Gem^{lite} scale to meet individual requirements by selecting from the parameters available in the menu.

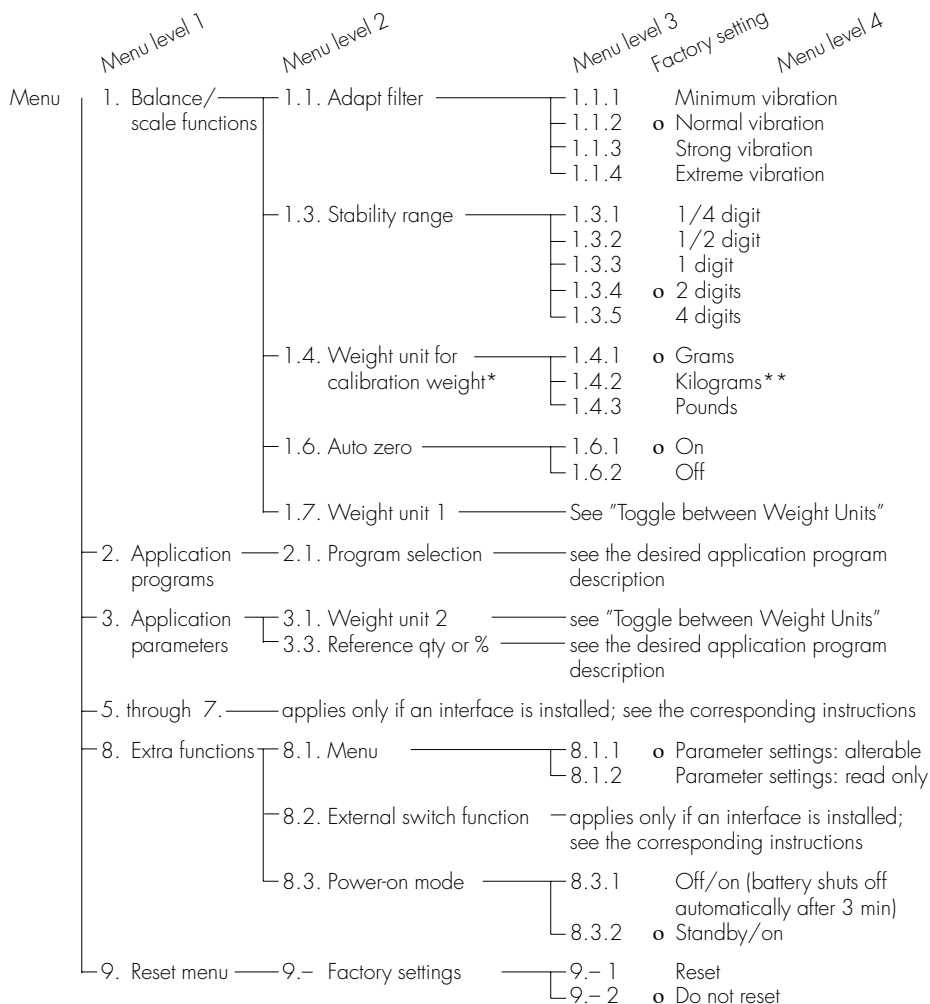
Example: Adapt the balance/scale to unstable ambient conditions:

Menu code 1 1 4

| Step | Key (or instruction) | Display |
|---|---|---|
| 1. Turn off the balance/scale |  | |
| 2. Turn the balance/scale back on; while all segments are displayed: |  |  |
| |  briefly | 1. |
| ○ To navigate within a menu level; the last menu option is followed by the first option |  repeatedly | 2. ... 9. 1. |
| 3. Select the 2nd menu level |  | 1. 1. |
| 4. Select the 3rd menu level |  | 1. 1. 2 ○ |
| 5. In Menu Level 3: Select the desired option |  repeatedly | 1. 1. 4 |
| 6. Confirm new setting; the "o" indicates the currently set option |  for 2 sec. | 1. 1. 4 ○ |
| ○ Select the next menu level (here: move from the 3rd to the 1st level) |  | 1. |
| ○ Set other menu codes, if desired |  ,  | |
| 7. Store parameter settings and exit operating menu or |  for 2 sec. |  |
| ○ Exit operating menu without storing changes |  | |
| > Restart the application | | 0.0 g |

Balance/Scale Operating Menu (Overview)

- o Factory setting
- User setting



* = only for BL models

** = not for models with a readability of 0.1 mg

Error Codes

Error codes are shown on the main display for approx. 2 seconds, after which the program automatically returns to the weighing mode.

| Display | Cause | Solution |
|--|--|--|
| No segments appear on the display | No AC power is available The AC adapter is not plugged in Battery is dead | Check the AC power supply Plug in the AC adapter Replace the battery Recharge the battery using an external charger |
| H | The load exceeds the balance/scale capacity | Unload the balance/scale |
| L | The weighing pan is not in place Something is touching the weighing pan | Place the weighing pan on the balance/scale Move the object that is touching the weighing pan |
| E 0 1 | Display capacity exceeded: Value to be output cannot be shown on the display | Decrease the weight on the balance/scale |
| E 02 | Calibration parameter requirement not met; e.g.: – balance/scale not zeroed – balance/scale is loaded | Calibrate only when zero is displayed Press [TARE] to tare the balance/scale Unload the balance/scale |
| E 09 | When gross value \leq zero, no tare | Tare the balance/scale |
| E 10 | The [TARE] key is blocked when there is data in the second tare memory (net-total) – only 1 tare function can be used at a time | Press [CF] to clear the tare memory and release the tare key |
| E 11 | Value input is not allowed for second tare memory | Press [TARE] |
| E 22 | Weight is too light or there is no sample on the balance/scale | Increase the reference quantity or sample amount |
| E 30 | Interface port for printer output is blocked | Contact your local Sartorius Service Center |
| Max. weighing capacity is less than indicated under "Specifications" | The balance/scale was turned on without the weighing pan in place | Place the weighing pan on the balance/scale and press [ON] to turn the balance/scale back on |
| The weight readout is obviously wrong | The balance/scale has not been calibrated/adjusted The balance/scale was not tared before weighing | Calibrate/adjust the balance/scale Tare before weighing |

If any other errors occur, please contact your local Sartorius Service Center.

Care and Maintenance

Service


Regular servicing by a Sartorius technician will extend the service life of your balance/scale and ensure its continued weighing accuracy. Sartorius can offer you service contracts, with your choice of regular maintenance intervals ranging from 1 month to 2 years. The frequency of the maintenance intervals depends on the user's operating conditions and the tolerance limits.

Repairs

Repair work must be performed by trained service technicians. Any attempt by untrained persons to perform repairs may lead to hazards for the user.

Cleaning

- ⚠ Disconnect the balance/scale from the AC adapter and unplug any interface cables that are connected to the balance/scale
- ⚠ Make sure that no liquid enters the balance/scale housing
- ⚠ Do not use any aggressive cleaning agents (solvents or similar agents)
- Clean the balance/scale using a piece of cloth which has been wet with a mild detergent (soap)
- After cleaning, wipe down the balance/scale with a soft, dry cloth



Removing and Cleaning the Weighing Pan:

- Lift up and remove the weighing pan together with the pan support by gripping them from under the shield ring. Make sure that you do not damage the weighing system in doing so.

Safety Inspection

If there is any indication that safe operation of the balance/scale with the AC adapter is no longer warranted:

- Turn off the power and disconnect the equipment from AC power immediately
- > Lock the equipment in a secure place to ensure that it cannot be used for the time being

Safe operation of the balance/scale with the AC adapter is no longer ensured when:

- there is visible damage to the AC adapter
- the AC adapter no longer functions properly
- The AC adapter has been stored for a relatively long period under unfavorable conditions

In this case, notify your nearest Sartorius Service Center or the International Technical Support Unit based in Goettingen, Germany. Maintenance and repair work may only be performed by service technicians who are authorized by Sartorius and who

- have access to the required maintenance manuals
- have attended the relevant service training courses

Instructions for Recycling the Packaging

To ensure adequate protection for safe shipment, your balance/scale has been packaged to the extent necessary using environmentally friendly materials. After successful installation of the balance/scale, you should return this packaging for recycling because it is a valuable source of secondary raw material.

For information on recycling options, including recycling of old weighing equipment, contact your municipal waste disposal center or local recycling depot.

Overview

Specifications

Basic^{lite} Series

| Model | | BL210S | BL120S | BL60S |
|--|--------|--|--------------------|--------------------|
| Weighing capacity | g | 210 | 120 | 60 |
| Readability | mg | 0.1 | 0.1 | 0.1 |
| Tare range (subtractive) | g | 210 | 120 | 60 |
| Repeatability | ≤±mg | 0.1 | 0.1 | 0.1 |
| Linearity | ≤±mg | 0.2 | 0.2 | 0.2 |
| Operating temperature range | | +10...+30°C (50°F–86°F) | | |
| Allowable ambient operating temperature | | +5...+40°C | | |
| Sensitivity drift within +10...+30°C | ≤±/K | 2·10 ⁻⁶ | 2·10 ⁻⁶ | 2·10 ⁻⁶ |
| Response time (average) | s | 3 | 3 | 3 |
| Adaptation to ambient conditions | | By selection of 1 of 4 optimized filter levels | | |
| Display update (depends on the filter level selected) | s | 0.1–0.4 | | |
| External calibration weight (of at least accuracy class...) | g | 200 (E2) | 100 (E2) | 50 (E2) |
| | lb | 0.4 (E2) | 0.2 (E2) | 0.1 (E2) |
| Net weight, approx. | kg/lb | 3.0/6.6 | 3.0/6.6 | 3.0/6.6 |
| Pan size | mm | 80 Ø | 80 Ø | 80 Ø |
| | inches | 3.3 Ø | 3.3 Ø | 3.3 Ø |
| Weighing chamber height | mm | 200 | 200 | 200 |
| | inches | 7.9 | 7.9 | 7.9 |
| Dimensions (WxDxH) | mm | 189x251x299 | | |
| | inches | 7.4x9.9x11.8 | | |
| AC power source/ power requirements | | AC adapter, 230 V or 115 V, +15%...–20% | | |
| Frequency | | 48–60 Hz | | |
| Power requirements, direct current | V | 10 to 20 | | |
| Power consumption (average) | W | 1 | 1 | 1 |
| Approx. hours of operation with: – 9-volt battery, approx. | h | – | – | – |
| – fully charged rechargeable battery | h | – | – | – |
| Hours of operation with the YRB08Z rechargeable battery pack | h | 20 | 20 | 20 |

Gem^{lite} Series

| Model | | GC503 | GC103 | GM1205 |
|--|--------------|--|----------------------------|---------------------------|
| Weighing capacity | | 505 ct/101 g | 105 ct/21 g | 1200 g |
| Readability | | 0.001 ct/0.2 mg | 0.001 ct/0.2 mg | 50 mg |
| Tare range (subtractive) | | 505 ct/101 g | 105 ct/21 g | 1200 g |
| Repeatability | ≤± | 0.001 ct/0.2 mg | 0.001 ct/0.2 mg | 50 mg |
| Linearity | ≤± | 0.002 ct/0.4 mg | 0.002 ct/0.4 mg | 100 mg |
| Operating temperature range | | +10...+30°C (50°F–86°F) | | |
| Allowable ambient operating temperature | | +5...+40°C | | |
| Sensitivity drift within +10...+30°C | ≤±/K | 2·10 ⁻⁶ | 2·10 ⁻⁶ | 2·10 ⁻⁵ |
| Response time (average) | s | 3 | 3 | 2 |
| Adaptation to ambient conditions | | By selection of 1 of 4 optimized filter levels | | |
| Display update (depends on the filter level selected) | s | 0.2–0.4 | 0.2–0.4 | 0.2–0.8 |
| External calibration weight (of at least accuracy class...) | g lb | 100 (F1) – | 20 (F1) – | 1000 (F2) – |
| Net weight, approx. | kg/lb | 2.8/6.2 | 2.8/6.2 | 1.4/3.1 |
| Pan size | mm inches | 80 Ø 3.3 Ø | 80 Ø 3.3 Ø | 174 x 143 6.9 x 5.6 |
| Weighing chamber height | mm inches | 133 5.2 | 133 5.2 | – – |
| Dimensions (WxDxH) | mm inches | 189x251x233 7.4x9.9x9.2 | 189x251x233 7.4x9.9x9.2 | 189x251x70 7.4x9.9x2.8 |
| AC power source/ power requirements | | AC adapter, 230 V or 115 V, +15%...–20% | | |
| Frequency | | 48–60 Hz | | |
| Power requirements, direct current | V | 10 to 20 | | |
| Power consumption (average) | W | 1 | 1 | 0.75 |
| Approx. hours of operation with: – 9-volt battery, approx. | h | – | – | 11 |
| – fully charged rechargeable battery | h | – | – | 2.5 |
| Hours of operation with the YRB08Z rechargeable battery pack | h | 20 | 20 | 25 |

Basic^{lite} Series and Gem^{lite} Series

| Model | | BL150S | BL1500S, GM1502 | BL610, GM612 | BL310, GM312 | GM212 | BL150, GM152 | BL6100, GM6101 |
|--|--------|--|----------------------|----------------------|--------------------|--------------------|--------------------|----------------------|
| Weighing capacity | g | 150 | 1500 | 610 | 310 | 210 | 150 | 6100 |
| Readability | g | 0.001 | 0.01 | 0.01 | 0.01 | 0.01 | 0.01 | 0.1 |
| Tare range (subtractive) | g | 150 | 1500 | 610 | 310 | 210 | 150 | 6100 |
| Repeatability | ≤±g | 0.0015 | 0.015 | 0.01 | 0.01 | 0.01 | 0.01 | 0.1 |
| Linearity | ≤±g | 0.003 | 0.03 | 0.02 | 0.02 | 0.02 | 0.02 | 0.2 |
| Operating temperature range | | +10...+30°C (50°F...86°F) | | | | | | |
| Allowable ambient operating temperature | | +5...+40°C | | | | | | |
| Sensitivity drift within +10...+30°C | ≤± /K | 3.3·10 ⁻⁶ | 3.3·10 ⁻⁶ | 0.5·10 ⁻⁵ | 1·10 ⁻⁵ | 1·10 ⁻⁵ | 2·10 ⁻⁵ | 0.5·10 ⁻⁵ |
| Response time (average) | s | 2.5 | 2.5 | 2 | 2 | 2 | 1.5 | 2 |
| Adaptation to ambient conditions | | By selection of 1 of 4 optimized filter levels | | | | | | |
| Display update (depends on the filter level selected) | s | 0.2–0.8 | | | | | | |
| External calibration weight (of at least accuracy class...) | g | 100 (F1) | 1000 (F1) | 500 (F2) | 100 (F2) | 100 (F2) | 100 (M1) | 5000 (F2) |
| | lb* | 0.2 (F1) | 2 (F1) | 1 (F2) | 0.2 (F2) | 0.2 (F2) | 0.2 (M1) | 10 (F2) |
| Net weight, approx. | kg | | | | | | | |
| | /lb | 1.6/3.5 | 1.4/3.1 | 1.1/2.4 | 1.1/2.4 | 1.1/2.4 | 1.1/2.4 | 1.4/3.1 |
| Pan size | mm | 100 Ø | 174x143 | 116 Ø | 116 Ø | 116 Ø | 116 Ø | 174x143 |
| | inches | 3.9 Ø | 6.9x5.6 | 4.6 Ø | 4.6 Ø | 4.6 Ø | 4.6 Ø | 6.9x5.6 |
| Dimensions (WxDxH) | mm | 189x251x70 (7.4x9.9x2.8 inches) | | | | | | |
| AC power source/ power requirements | | AC adapter, 230 V or 115 V, +15%...– 20% | | | | | | |
| Frequency | | 48–60 Hz | | | | | | |
| Power requirements, direct current | V | 10 to 20 | | | | | | |
| Power consumption (average) | W | 0.75 | | | | | | |
| Approx. hours of operation with: – 9-volt battery, approx. h | – | – | – | 11 | 11 | 11 | 11 | 11 |
| – fully charged rechargeable battery h | – | – | – | 2.5 | 2.5 | 2.5 | 2.5 | 2.5 |
| Hours of operation with the YRB08Z rechargeable battery pack | h | 25 | | | | | | |

* = only for BL models

Basic^{lite} und Gem^{lite} Serie

| Model | | BL3100 GM3101 | BL1500 | BL600, GM601 | BL12 | BL6 | BL3 |
|--|-----------|--|--------------------|--------------------|----------------------|--------------------|---------------------|
| Weighing capacity | g | 3100 | 1500 | 610 | 12000 | 6000 | 3000 |
| Readability | g | 0.1 | 0.1 | 0.1 | 1 | 1 | 1 |
| Tare range (subtractive) | g | 3100 | 1500 | 610 | 12 | 6 | 3 |
| Repeatability | ≤±g | 0.1 | 0.1 | 0.1 | 1 | 1 | 1 |
| Linearity | ≤±g | 0.2 | 0.2 | 0.2 | 2 | 2 | 2 |
| Operating temperature range | | +10...+30°C (50°F...86°F) | | | | | |
| Allowable ambient operating temperature | | +5...+40°C | | | | | |
| Sensitivity drift within +10...+30°C | ≤±/K | 1·10 ⁻⁵ | 2·10 ⁻⁵ | 5·10 ⁻⁵ | 2.5·10 ⁻⁵ | 5·10 ⁻⁵ | 10·10 ⁻⁵ |
| Response time (average) | s | 2 | 1.5 | 1.5 | 1.5 | 1.5 | 1.5 |
| Adaptation to ambient conditions | | By selection of 1 of 4 optimized filter levels | | | | | |
| Display update (depends on the filter level selected) | s | 0.2–0.8 | | | | | |
| External calibration weight (of at least accuracy class...) | kg lb* | 1 (F2) 2 (F2) | 1 (M1) 2 (M1) | 0.5 (M1) 1 (M1) | 5 (M1) 10 (M1) | 5 (M1) 10 (M1) | 1 (M1) 2 (M1) |
| Net weight, approx. | kg/lb | 1.4/3.1 | | | | | |
| Pan size | mm | 174x143 (6.9x5.6 inches) | | | | | |
| Dimensions (WxDxH) | mm | 189x251x70 (7.4x9.9x2.8 inches) | | | | | |
| AC power source/ power requirements | | AC adapter, 230 V or 115 V, +15%...– 20% | | | | | |
| Frequency | | 48–60 Hz | | | | | |
| Power requirements, direct current | V | 10 to 20 | | | | | |
| Power consumption (average) | W | 0.75 | | | | | |
| Approx. hours of operation with: – 9-volt battery, approx. | h | 11 | | | | | |
| – fully charged rechargeable battery | h | 2.5 | | | | | |
| Hours of operation with the YRB08Z rechargeable battery pack | h | 25 | | | | | |

* = only for BL models

Accessories (Options)

| Product | Order No. | Product | Order No. |
|---|-----------|---|----------------------|
| Interface port, installation kit | YDO02BL | Dust cover , for use during weighing | |
| Data printer | YDP04 | – for models with a rectangular weighing pan | YDC01BL |
| Data printer with date/time, statistics evaluation and transaction counter functions and LCD (data interface required) | YDP03-OCE | – for models with a round weighing pan | YDC02BL |
| Paper (5 rolls) | 6906937 | Attaching the dust cover to models with a glass draft shield: | |
| Remote display (data interface required) | | – Remove adhesive strip from balance/scale housing | |
| – reflective | YRD12Z | – Place dust cover on balance/scale | |
| – for overhead projectors, transmissive | YRD13Z | – Stick adhesive strip on dust cover | |
| External rechargeable battery pack YRB08Z with external battery charger (hours of operation: 20 or 40, depending on balance/scale model) | | Gem trays | |
| SartoWedge data transfer software YSW01 for on-line storage of weighing data | | – 300 ml, weight: 86 g, stainless steel | 6407 |
| Interface cable 7357312 for connecting a PC; 25-pin | | – 1000 ml, wt.: 240 g, stainless steel | 641211 |
| Universal remote control switch: (data interface required) | | – 300 ml, wt.: 22 g, aluminum | 69641304 |
| Foot switch with T-connector YFS01 | | – 110 ml, 90 Ø mm, aluminum | YWP02G |
| Hand switch with T-connector YHS01 | | – 270 ml, wt.: 62 g, 137 Ø mm stainless steel | YWP03G |
| T-connector YTC01 for connecting 2 peripheral devices (data interface required) | | Calibration weights | |
| Carrying case | | – for BL210S (200 g; E2) | YCW5228 |
| – for models with a readability ≥ 1 mg | YDB01BL | – for BL120S, BL150S, GC503* (100 g; E2) | YCW5128 |
| – for models BL210S, BL120S, BL60S | YDB02BL | – for GC103 (20 g; F1) | YCW4238 |
| | | – for BL60S (50 g; E2) | YCW4528 |
| | | – for the BL150, BL310, GM512, GM312 (100 g; F2) | YCW5148 |
| | | – for the BL610, BL600, GM612 (500 g; F2) | YCW5548 |
| | | – for the BL1500S, GM1502 (1 kg; F1) | YCW6138 |
| | | – for the BL1500, BL3100, BL3, GM3101, GM1205 (1 kg; F2) | YCW6148 |
| | | – for the BL6100, BL6, BL12, GM6101 (5 kg; F1) or alternative | YCW6538 YSS653-00 |
| | | * = F1 100-g weight supplied with the GC503 scale | |

CE Marking

The CE marking affixed to the equipment indicates that the equipment meets the requirements of the following Directive(s):

Council Directive 89/336/EEC "Electromagnetic compatibility (EMC)"

Applicable European Standards:

Limitation of emissions:

EN 50081-1 Residential, commercial and light industry

EN 50081-2 Industrial environment

Defined immunity to interference:

EN 50082-1 Residential, commercial and light industry

EN 50082-2 Industrial environment

Important Note:

The operator shall be responsible for any modifications to Sartorius equipment and for any connections of cables or equipment not supplied by Sartorius and must check and, if necessary, correct these modifications and connections. On request, Sartorius will provide information on the minimum operating specifications (in accordance with the Standards listed above for defined immunity to interference).

Council Directive 73/23/EEC

"Electrical equipment designed for use within certain voltage limits"

Applicable European Standards:

EN 60950 Safety of information technology equipment including electrical business equipment

EN 61010 Safety requirements for electrical equipment for measurement, control and laboratory use
Part 1: General requirements

If you use electrical equipment in installations and under ambient conditions requiring higher safety standards, you must comply with the provisions as specified in the applicable regulations for installation in your country.

Sartorius AG

✉ 37070 Goettingen, Germany

🏠 Weender Landstrasse 94-108, 37075 Goettingen, Germany

☎ (+49/551) 308-0, 📠 (+49/551) 308-3289

Internet: <http://www.sartorius.com>

Copyright by Sartorius AG, Goettingen, Germany.

All rights reserved. No part of this publication may be reprinted or translated in any form or by any means without the prior written permission of Sartorius AG.

The status of the information, specifications and illustrations in this manual is indicated by the date given below. Sartorius AG reserves the right to make changes to the technology, features, specifications and design of the equipment without notice.

Status: January 2001, Sartorius AG, Goettingen, Germany